

इंटरनेट

मानक

Disclosure to Promote the Right To Information

Whereas the Parliament of India has set out to provide a practical regime of right to information for citizens to secure access to information under the control of public authorities, in order to promote transparency and accountability in the working of every public authority, and whereas the attached publication of the Bureau of Indian Standards is of particular interest to the public, particularly disadvantaged communities and those engaged in the pursuit of education and knowledge, the attached public safety standard is made available to promote the timely dissemination of this information in an accurate manner to the public.

“जानने का अधिकार, जीने का अधिकार”

Mazdoor Kisan Shakti Sangathan

“The Right to Information, The Right to Live”

“पुराने को छोड़ नये के तरफ”

Jawaharlal Nehru

“Step Out From the Old to the New”

IS 15758-1 (2007): Textiles - Protective clothing, Part 1:
Method of determining of heat transmission on exposure to
flame [TXD 32: Textiles Protective Clothing]



“ज्ञान से एक नये भारत का निर्माण”

Satyanarayan Gangaram Pitroda

“Invent a New India Using Knowledge”



“ज्ञान एक ऐसा खजाना है जो कभी चुराया नहीं जा सकता है”

Bhartrhari—Nitiśatakam

“Knowledge is such a treasure which cannot be stolen”

BLANK PAGE



भारतीय मानक
वस्त्रादि — सुरक्षा वस्त्र

भाग 1 लौ के संपर्क पर उष्मा के संचारण की विधि ज्ञात करना

Indian Standard
TEXTILES — PROTECTIVE CLOTHING
**PART 1 METHOD OF DETERMINING OF HEAT TRANSMISSION ON
EXPOSURE TO FLAME**

ICS 13.340.10

© BIS 2007

BUREAU OF INDIAN STANDARDS
MANAK BHAVAN, 9 BAHADUR SHAH ZAFAR MARG
NEW DELHI 110002

August 2007

Price Group 5

NATIONAL FOREWORD

This Indian Standard (Part 1) which is identical with ISO 9151 : 1995 'Protective clothing against heat and flame — Determination of heat transmission on exposure to flame' issued by the International Organization for Standardization (ISO) was adopted by the Bureau of Indian Standards on the recommendation of the Chemical Methods of Test Sectional Committee and approval of the Textile Division Council.

The conditioning temperature of $20 \pm 2^{\circ}\text{C}$ as specified in International Standard is not suitable for tropical countries like India where the atmospheric temperature is normally much higher than 20°C . It is almost impossible to maintain this temperature specially during summer when the atmospheric temperature rises even up to 50°C . In view of the above, IS 6359 : 1971 'Method for conditioning of textiles' specifies a temperature of $27 \pm 2^{\circ}\text{C}$ for conditioning of the test specimens for the tropical countries like India. This standard is being followed in testing of textiles and other products since decades.

The text of ISO Standard has been approved as suitable for publication as an Indian Standard without deviations. Certain conventions are, however, not identical to those used in Indian Standards. Attention is particularly drawn to the following:

- a) Wherever the words 'International Standard' or 'European Standard' appear referring to this standard, they should be read as 'Indian Standard'.
- b) Comma (,) has been used as a decimal marker, while in Indian Standards, the current practice is to use a point (.) as the decimal marker.

In reporting the results of a test or analysis made in accordance with this standard, if the final value, observed or calculated, is to be rounded off, it shall be done in accordance with IS 2 : 1960 'Rules for rounding off numerical values (*revised*)'.

Indian Standard
TEXTILES — PROTECTIVE CLOTHING
PART 1 METHOD OF DETERMINING OF HEAT TRANSMISSION ON
EXPOSURE TO FLAME

1 Scope

This International Standard specifies a method for comparing the heat transmission through materials or material assemblies used in protective clothing. Materials are ranked by calculation of a heat transfer index, which is an indication of the relative heat transmission under the specified test conditions. The heat transfer index should not be taken as a measure of the protection time given by the tested materials under actual use conditions.

2 Normative references

The following standards contain provisions which, through reference in this text, constitute provisions of this International Standard. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this International Standard are encouraged to investigate the possibility of applying the most recent editions of the standards indicated below. Members of IEC and ISO maintain registers of currently valid International Standards.

ISO 139:1973, *Textiles — Standard atmospheres for conditioning and testing*.

IEC 584-1:1977, *Thermocouples — Part 1: Reference tables*.

3 Definitions

For the purposes of this International Standard, the following definitions apply.

3.1 test specimen: All the layers of fabric or other materials arranged in the order and orientation as used in practice and including undergarments.

3.2 incident heat flux density: Amount of energy incident per unit time on the exposed face of the specimen, expressed in kilowatts per square metre (kW/m^2).

3.3 heat transfer index (flame): Whole number calculated from the mean time in seconds to achieve a temperature rise of $(24 \pm 0,2)^\circ\text{C}$ when testing by this method using a copper disc of mass $(18 \pm 0,05)\text{ g}$ and a starting temperature of $(25 \pm 5)^\circ\text{C}$.

4 Principle

A horizontally oriented test specimen is partially restrained from moving and subjected to an incident heat flux of 80 kW/m^2 from the flame of a gas burner placed beneath it. The heat passing through the specimen is measured by means of a small copper calorimeter on top of and in contact with the specimen.

The time, in seconds, for the temperature in the calorimeter to rise $(24 \pm 0,2)^\circ\text{C}$ is recorded. The mean result for three test specimens is calculated as the "heat transfer index (flame)".

5 Apparatus

The apparatus consists of

- a gas burner;
- a copper disc calorimeter;
- a specimen support frame;
- a calorimeter location plate;

- a support stand;
- suitable measuring equipment;
- a template.

5.1 Gas burner.

A flat topped Meker burner with a perforated top area of (38 ± 2) mm diameter and a jet suitable for propane gas shall be used.

Commercial grade propane shall be used with the flow being controlled by a fine control valve and flowmeter.


5.2 Copper disc calorimeter, consisting of a disc of copper of at least 99 % purity, having a diameter of 40 mm and thickness 1,6 mm, and a mass of 18 g. The disc shall be accurately weighed before assembly.

A copper-constantan thermocouple, with an output in millivolts complying with IEC 584-1, is mounted on the copper disc as shown in figure 1. The constantan wire shall be attached to the centre of the disc and the copper wire shall be attached as near the circumference as possible but so as not to interfere with mounting the disc in the block. The diameter of both wires shall be 0,26 mm or less and only the length attached to the disc shall be bared.

The calorimeter is located in a mounting block which shall consist of a 89 mm diameter circular piece of asbestos-free noncombustible heat insulating board of nominal thickness 13 mm. The thermal characteristics shall comply with the following specification:

Density	$(750 \pm 50) \text{ kg/m}^3$
Thermal conductivity	$0,18 \text{ W/(m}\cdot\text{K)} \pm 10 \%$


A circular cavity is machined in the centre of the block to accommodate the disc and an air gap, as shown in figure 2. The disc is bonded in position around its circumference with an adhesive capable of withstanding temperatures of about 200 °C. The face of the copper disc shall be flush with the surface of the mounting block. It shall also be coated with a thin layer of an optically black paint having a coefficient of absorption, α , greater than 0,9 (see annex A).

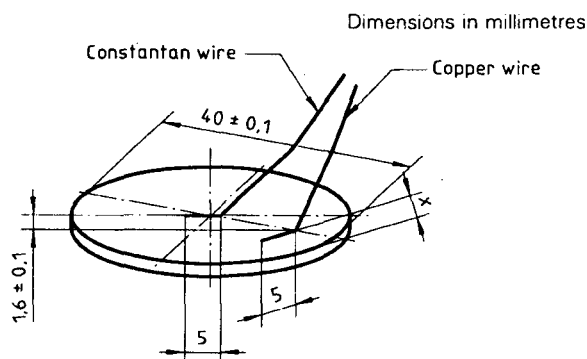

NOTES

- 1 $2 \text{ mm} \leq x \leq 5 \text{ mm}$ so as not to interfere with the seating of disc in the mounting block but still as near the edge as possible.
- 2 The wires shall be attached to the disc by soft solder using the minimum quantity necessary.

Figure 1 — Calorimeter

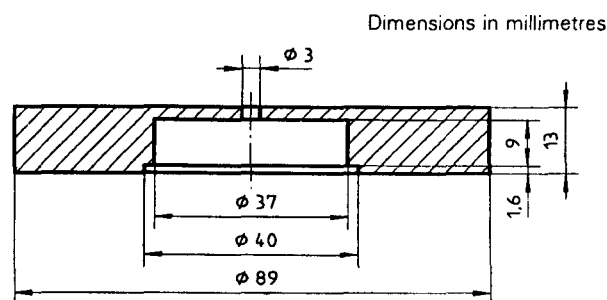

Construction material: Monolux 500 (cape boards) or equivalent.

Figure 2 — Calorimeter mounting block

5.3 Specimen support frame, consisting of a piece of copper 150 mm square and 1,6 mm thick with a 50 mm square hole in its centre (see figure 3).

5.4 Calorimeter location plate, made from a piece of aluminium 149 mm square and 6 mm thick and having a circular hole 90 mm in diameter located centrally (see figure 4). The plate shall weigh $(264 \pm 13) \text{ g}$.

5.5 Support stand, used to locate the specimen support frame relative to the burner. The top face of the specimen support frame shall be 50 mm above and parallel with the top face of the burner, with the axis of the burner aligned with the centre of the opening in the support frame (see figure 5).

It is convenient to have a shutter between the burner and the specimen support frame. The shutter shall open completely in less than 0,2 s and shall be operated immediately after placing the burner in position. It is useful if the positioning of the burner, or the opening of the shutter, if fitted, can be used to record the start of the exposure automatically.

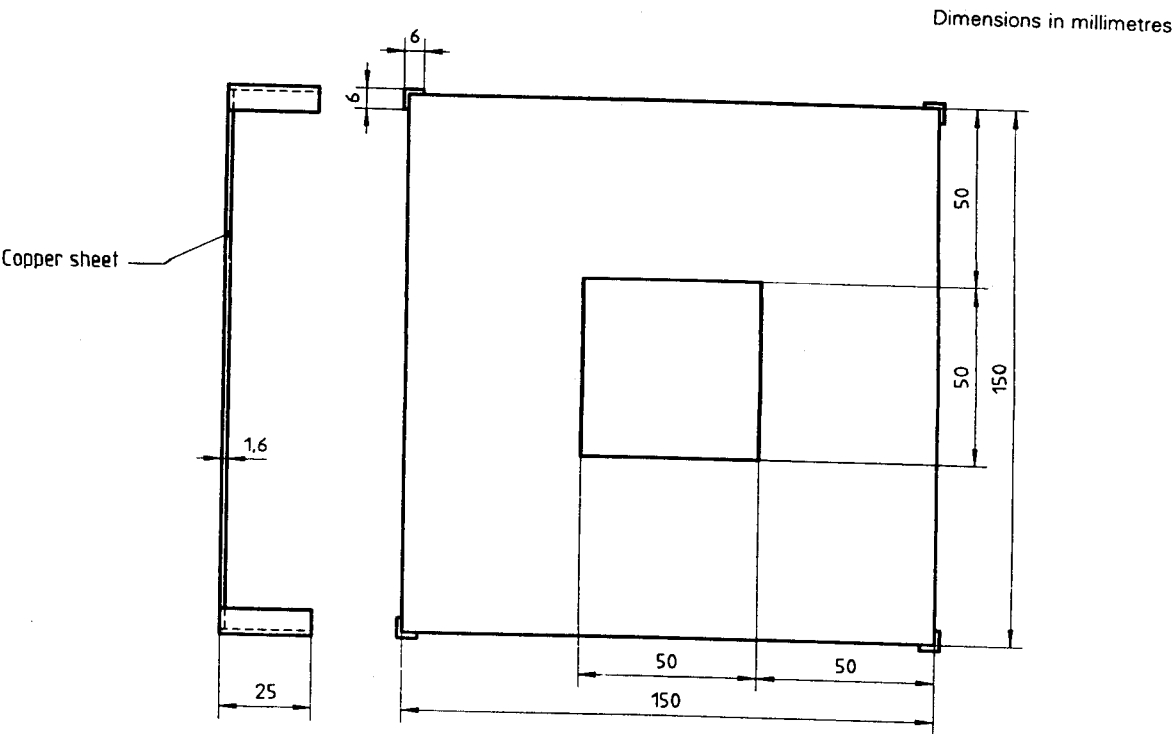


Figure 3 — Specimen support frame

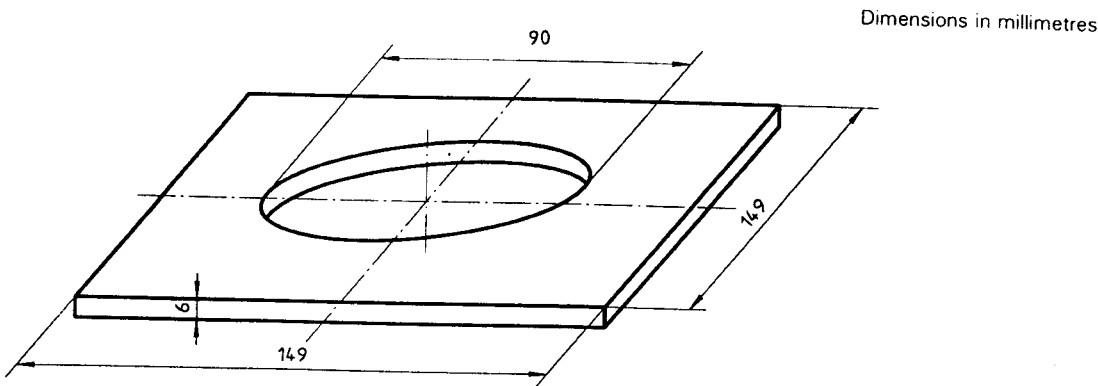


Figure 4 — Calorimeter location plate

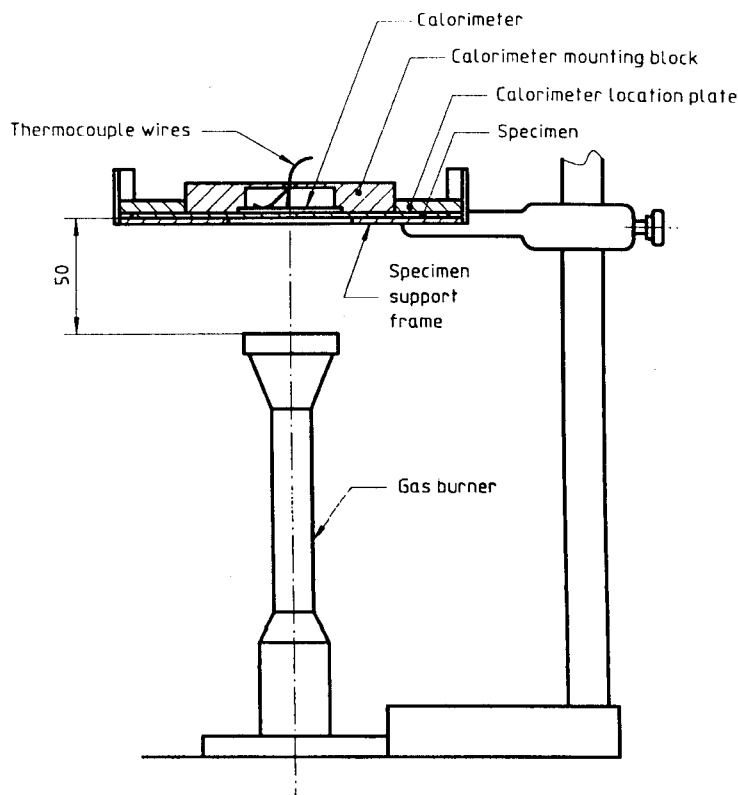


Figure 5 — Support stand

5.6 Recorder.

To enable the absolute temperature of the copper disc to be determined, the thermocouple should be connected to either an ice junction or a commercial reference junction. The voltage signal from the thermocouple shall be connected to either a suitable potentiometric chart recorder or programmable data recorder. The recorder shall enable voltages to be read to 10 μV and times to 0,2 s.

5.7 Flat rigid template, with dimensions 140 mm $\times$ 140 mm.

6 Precautions

Perform the test in a hood or ventilated area to carry away the fumes. It may be necessary to turn off the exhaust or to shield the apparatus during the test so as not to disturb the flame.

The equipment becomes hot during testing and some test materials may melt or drip. Use protective gloves when handling hot objects.

Keep combustible materials away from the burner. Ensure that the solvent used for cleaning the calorimeter is kept away from hot surfaces and naked flames.

7 Sampling

7.1 Specimen dimensions

The specimens shall have the dimensions 140 mm $\times$ 140 mm and shall be taken from points more than 50 mm from the edge of the pieces of the material, in an area free from defects. Composite specimens shall reproduce the arrangement in which the layers are used in practice.

The specimen shall be marked out using the template (see 5.7).

7.2 Number of specimens

A minimum of three specimens shall be tested for each material or assembly of materials.

8 Conditioning and testing atmospheres

8.1 Conditioning atmosphere

Prior to testing, the specimens shall be conditioned for at least 24 h at a temperature of $(20 \pm 2)^\circ\text{C}$ and a relative humidity of $(65 \pm 2)\%$ (see ISO 139). If testing is not carried out immediately after conditioning, place the conditioned test specimens in a sealed container. Begin testing of each specimen within 3 min of removing it from the conditioning atmosphere or sealed container.

8.2 Testing atmosphere

Perform the tests in an atmosphere having a temperature of 10°C to 30°C and a relative humidity of 15 % to 80 % and which is free from draughts.

9 Test procedure

9.1 Preparation and calibration

9.1.1 Preliminary measures

Position the support frame on the support stand so that the top surface on which the specimen is placed is 50 mm above the top face of the burner. It is suggested that a guide and stops be used to enable the burner to be positioned quickly with its axis in line with the centre of the specimen.

Place the burner to one side, activate and ignite the gas supply, and allow several minutes for flame stabilization.

Connect the thermocouple to the cold junction, and connect the output voltage into the recording device.

Before every incident heat flux density regulation or specimen evaluation, the copper disc temperature should be in a relatively steady state and within $\pm 2^\circ\text{C}$ of ambient temperature. Cooling may be accelerated by the use of any dry, chilled heat sink, or by forced air draught. Alternatively, a number of calorimeter units may be rotated. Heating may be achieved by contact of the palm of the hand with the copper disc or by short exposure to the burner flame.

WARNING — On no account shall the calorimeter mounting block be allowed to come into contact with water. If this occurs accidentally it shall be dried out thoroughly before further use.

9.1.2 Regulation of the incident heat flux density

The gas flowrate and burner setting will vary with the individual combination used, and regulation of the settings for one or both will be necessary during initial installation and from time to time during testing. The correct flux should be achieved from a flame with clearly defined stable light blue cones firmly positioned on the burner grid with a large diffuse bluish flame above.

The flame setting is confirmed by measuring the heat flux density with the calorimeter.

Place the calorimeter location plate on the specimen support frame. Place the calorimeter in the hole in the locating plate with the copper disc facing downwards.

Select the required rate of travel of the recording device, and slide the burner quickly and deliberately under the calorimeter until it locates against its stops. If a shutter is used, open the shutter (see 5.5).

Allow the burner to remain in position for about 10 s.

Withdraw the burner or close the shutter.

The recorded output should show a short nonlinear temperature-time region just after the start of the exposure, followed by a linear region which continues until exposure ceases. Refer to standard thermocouple electromotive force tables to determine the rate of rise of temperature in degrees Celsius per second of this linear region. The heat flux density, Q (in kW/m^2) is then determined from the following equation:

$$Q = \frac{Mc_p R}{A}$$

where

- M is the mass of the copper disc in kilograms;
- c_p is the specific heat capacity of the copper [$= 0,385 \text{ kJ/(kg}\cdot^\circ\text{C)}$];
- R is the rate of rise in disc temperature in the linear region in degrees Celsius per second;
- A is the disc area in square metres.

The heat flux density determined by this procedure shall be within $\pm 5\%$ of the specified 80 kW/m^2 . Adjust the gas flowrate if required, and repeat until three consecutive values are obtained which fall within the required limits.

9.2 Test specimen mounting

9.2.1 Place the outermost layer of the specimen face downwards on the specimen support frame (see 5.3). Place the location plate (see 5.4) on top of the specimen.

9.2.2 If the specimen consists of more than one layer and the layers are not attached to one another, remove the location plate and mount each successive layer in the order and orientation as used in the assembly. Use the weight of the location plate, with no additional pressure, to press each layer into contact with the previous layer.

9.2.3 After the last (innermost) layer has been mounted, replace the location plate and place the calorimeter in the hole in the location plate so that the copper disc is in contact with the top of the innermost layer.

9.3 Test specimen exposure

9.3.1 Slide the burner quickly and deliberately into position. Immediately move the shutter, if fitted, from below the specimen. Start the recording device simultaneously with the exposure of the specimen to the burner flame or mark the start of the exposure with the recorder already running, depending on the equipment used.

9.3.2 Allow the test to continue until a temperature rise of $(24 \pm 0,2) ^\circ\text{C}$ is observed. Observe and note any changes in specimen appearance during the test, e.g. shrinkage, scorching, charring, holing, glowing, melting or dripping. Replace the shutter, if fitted, and withdraw the burner. Switch off the recorder.

9.3.3 Remove the calorimeter and clean off any combustion products whilst it is still hot (see clause 6). Cool to within $\pm 2 ^\circ\text{C}$ of ambient temperature.

If the remaining deposit on the calorimeter is thick or uneven, if the black coating has deteriorated, or if the copper is exposed, the calorimeter disc shall be cleaned (see annex A) and repainted (see 5.2). At least one calibration run (see 9.1.2) shall be carried out with the recoated calorimeter before testing further specimens.

9.3.4 Measure the time in seconds for a temperature rise in the calorimeter of $(24 \pm 0,2) ^\circ\text{C}$ (see annex C).

9.3.5 Repeat the procedure with two more specimens. Calculate the heat transfer index as the mean of the times taken for a temperature rise of $(24 \pm 2) ^\circ\text{C}$, to the nearest whole number.

NOTE 1 It is also possible to measure the time in seconds for a temperature rise of $(12,0 \pm 0,1) ^\circ\text{C}$, corresponding to a thermocouple output increase of 0,5 mV using an 18 g calorimeter. This measurement can be used to determine to what extent heat transfer is delayed or reduced. However, it should be stressed that the times measured have only a limited accuracy and do not necessarily relate to protection times under actual use conditions.

10 Test report

The test report shall contain the following particulars:

- a) name of test laboratory;
- b) date;
- c) reference to this International Standard;
- d) identification reference of the materials tested;
- e) description of the test materials and the arrangement in which they were tested, if possible details of generic names, mass per unit area and thickness under no pressure and under the pressure of the location plate should be given;
- f) the time in seconds for a $24 ^\circ\text{C}$ temperature rise for each specimen tested and the heat transfer index calculated from these individual results;
- g) if requested, the time in seconds for a $12 ^\circ\text{C}$ temperature rise for each specimen tested may also be reported;
- h) description of any changes in appearance of the specimens;
- i) a statement as follows: "These results have been obtained by a test method intended solely to rank the material and are not necessarily applicable to actual fire conditions."

Annex A

(informative)

Availability of materials

The following are examples of sources of materials specified in this International Standard. Equally suitable alternatives are available from other sources. This information is given for the convenience of users of this International Standard and does not constitute an endorsement by ISO of these products.

Gas burner (5.1)

Fisher Burner model 3-902 P.

Fisher Scientific Company,
711 Forbes Ave.,
Pittsburg, PA 15219,
USA

Müller-Scherr,
Laborausrüstungsgesellschaft m.b.H. & Co. KG,
Leopold-Hasner-Strasse 36,
A-4020 Linz,
Austria

Insulating board (5.2)

Monolux 500.

Cape Boards & Panels Ltd.
Iver Lane,
Uxbridge UB80 2JQ,
England

Black paint (5.2)

Nextel Velvet Coating Black 2010.

3M UK Ltd.
P.O. Box 38, Yeoman House,
63 Croydon Road,
Penge, London SE20 7TR,
England

Calorimeter cleaning liquid (9.3.3)

A mixture of three parts 1,1,1-trichloroethane and one part ethanol by volume has been found suitable.

Calorimeter paint remover (9.3.3)

Acetone.

Annex B
(informative)

Specimen test report form

Tests carried out in accordance with ISO 9151

Test laboratory

Reference No. Date

Test materials	Type	Mass/unit area g/m ²	Thickness mm	
			No pressure	Under location plate
Layer 1 (outer)				
2				
3				
4				
5				

Test results

Incident heat flux kW/m²

Specimen	Time for 24 °C temperature rise
1	
2	
3	
	Heat transfer index

Observations on specimen appearance:

.....
.....

These results have been obtained by a test method aimed solely at ranking the materials tested and are not necessarily applicable to actual fire conditions.

Annex C
(informative)

Significance of the heat transfer test

The heat transfer index (HTI) provides a means of ranking the ability of clothing assemblies to delay the transfer of heat from a flame. It is derived from the time in seconds to achieve a 24 °C temperature rise under the specified test conditions, which corresponds to a thermocouple output increase of $(1 \pm 0,01) \text{ mV } (\pm 10 \text{ } \mu\text{V})$ and a total heat transfer of $(132,3 \pm 1,1) \text{ kJ/m}^2$.

The heat transfer through clothing is dependent on the thickness of the clothing assembly including any air gaps. The HTI is determined with the specimen compressed under a standard load so as to minimize any air gaps. Thicker clothing gives better protection and gives higher HTI values but with increased variability.

The heat transfer index should not be regarded as the time for which the clothing will provide protection against a flame. Under actual use conditions, the severity of the flame and the compression of the clothing are not constant and can vary considerably from the standard test conditions. The performance of wet clothing may differ from the performance of the dry test specimen.

An interlaboratory trial was carried out in 1989 testing 18 single or multilayer assemblies in five laboratories. A further interlaboratory trial in 1991 involved seven single or multilayer assemblies tested in seven different laboratories. The following formulae for repeatability and reproducibility were derived from this latest trial.

Repeatability = $0,19 + 0,055 \text{ (mean)}$
Reproducibility = $1,21 + 0,12 \text{ (mean)}$

The performance of the materials tested in these trials could be divided into five bands, as shown in table C.1.

Table C.1 illustrates how adding extra layers increases the HTI value. Thick materials, particularly those containing large volumes of entrapped air, are especially effective. The suggested limits for the different bands are based on the performance of actual materials and allow for the variability between laboratories.

The midpoints of each band are based on frequently occurring values and the band widths are twice the reproducibility based on this midpoint value. If performance levels are set too close to the formal value, different laboratories will give different classifications.

In this proposed classification, any test assembly giving results which fall on the limit of a particular band ought to be retested and classification based on a minimum of two sets of results falling within the same band. Assemblies which give results which differ by less than the reproducibility for the band should not be regarded as being significantly different. It is possible to determine the heat transfer index (HTI) (24-12) as an additional factor in order to distinguish between different materials. However, this parameter is also subject to poor reproducibility and to rounding errors.

Table C.1

Band	HTI limits	Typical assembly	Comments	Reproducibility
1	3 to 6	Single layer	Most single-layer fabrics give results of 4 or 5	1,7
2	7 to 12	Double layer, thick single	Covers a wide range of normal multilayer apparel	2,3
3	13 to 20	Triple layer, thick double	Specialist firefighting clothing has HTI about 16	3,2
4	21 to 30	Very thick	Specialist heat protective clothing	4,3
5	≥ 31	Extremely thick	Very special applications	—

Bureau of Indian Standards

BIS is a statutory institution established under the *Bureau of Indian Standards Act*, 1986 to promote harmonious development of the activities of standardization, marking and quality certification of goods and attending to connected matters in the country.

Copyright

BIS has the copyright of all its publications. No part of these publications may be reproduced in any form without the prior permission in writing of BIS. This does not preclude the free use, in course of implementing the standard, of necessary details, such as symbols and sizes, type or grade designations. Enquiries relating to copyright be addressed to the Director (Publications), BIS.

Review of Indian Standards

Amendments are issued to standards as the need arises on the basis of comments. Standards are also reviewed periodically; a standard along with amendments is reaffirmed when such review indicates that no changes are needed; if the review indicates that changes are needed, it is taken up for revision. Users of Indian Standards should ascertain that they are in possession of the latest amendments or edition by referring to the latest issue of 'BIS Catalogue' and 'Standards: Monthly Additions'.

This Indian Standard has been developed from Doc: No. TX 05 (0765).

Amendments Issued Since Publication

Amendment No.	Date of Issue	Text Affected

BUREAU OF INDIAN STANDARDS

Headquarters:

Manak Bhavan, 9 Bahadur Shah Zafar Marg, New Delhi 110 002

Telephones: 2323 0131, 2323 3375, 2323 9402

Website: www.bis.org.in

Regional Offices:

Central : Manak Bhavan, 9 Bahadur Shah Zafar Marg
NEW DELHI 110 002

Telephones

{ 2323 7617
2323 3841

Eastern : 1/14, C.I.T. Scheme VII M, V.I.P. Road, Kankurgachi
KOLKATA 700 054

{ 2337 8499, 2337 8561
2337 8626, 2337 9120

Northern : SCO 335-336, Sector 34-A, CHANDIGARH 160 022

{ 260 3843
260 9285

Southern : C.I.T. Campus, IV Cross Road, CHENNAI 600 113

{ 2254 1216, 2254 1442
2254 2519, 2254 2315

Western : Manakalaya, E9 MIDC, Marol, Andheri (East)
MUMBAI 400 093

{ 2832 9295, 2832 7858
2832 7891, 2832 7892

Branches: AHMEDABAD. BANGALORE. BHOPAL. BHUBANESHWAR. COIMBATORE. FARIDABAD.
GHAZIABAD. GUWAHATI. HYDERABAD. JAIPUR. KANPUR. LUCKNOW. NAGPUR.
PARWANOO. PATNA. PUNE. RAJKOT. THIRUVANANTHAPURAM. VISAKHAPATNAM.